



STEP 1: CLEANING




Clean the external parts of the Coriolis Compact using a wipe soaked in a solution of water and surfactants.



Wipe the entire unit using a soft cloth.

STEP 2: DECONTAMINATION

For samples collected from an area contaminated with biological agents

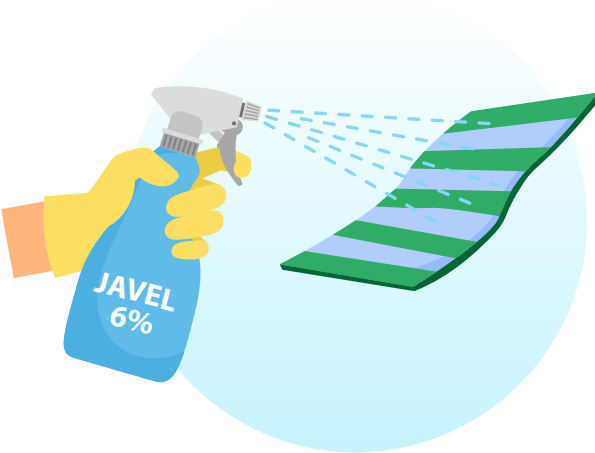

Spray 6% bleach solution onto a soft cloth.



Wipe the entire unit using the soft cloth. Incubate for 30 minutes.



Rinse thoroughly with fresh water.



Wipe the entire unit using another soft cloth.